

# Certificate of testing

## Crash Test according to ISO 7176-19 - 2008

### Wheeled mobility devices for use in motor vehicles

This report serves solely as documentation for the test results. The tested objects have been selected by the client with out the assistance of Dahl Engineering.

<b>Assignment:</b>	Crash testing of wheel chair and WTORS according to ISO 7176-19 annex A and B
<b>Date of testing:</b>	27 February 2018
<b>Test object:</b>	Medema mini crosser X model
<b>Mass of wheelchair:</b>	160kg
<b>Serial no:</b>	not informed
<b>WTORS:</b>	Dahl WTORS, meeting the requirements set out in clause 4.1 Wheelchair restraint – 4 p. Heavy duty tie down straps Occupant restraint – Dahl 3point seat belt #500984
<b>Test dummy:</b>	Hybrid II 50% dummy with mass of 77 Kg.
<b>Measuring:</b>	Accelerometers mounted on the crash test sled measured the deceleration.
<b>Photografi:</b>	The test was filmed with a high speed camera at 500 fps. Still pictures, pre and post-test.

### Test results

<b>Sled deceleration and speed:</b>	See page with plotted graph and speed
-------------------------------------	---------------------------------------

## Test Results

Section	Details	X if correct
<b>5.21</b>	<b>During the test</b>	
(a)	<b>Horisontal excursion limits</b>	
	Wheelchair point P $\leq$ 200 mm [Xwc]	48
	ATD knee $\leq$ 375 mm[Xknee]	157
	ATD front of head $\leq$ 650 mm [XheadF]	366
	ATD rear of head $\leq$ - 450 [XheadR]	-275
(b)	The knee excursion exceeded the wheelchair P point excursion	X
(c)	(Batteries on powered wheelchairs) did not move completely outside the wheelchair footprint or move into the wheelchair user's space or contact with ADT legs	X
<b>5.2.2</b>	<b>After the test</b>	
(a)	The wheelchair remained in an upright position on the platform	X
	The ADT remained in the wheelchair with its torso at an angle of not more than 45° to the vertical, when viewed from any direction	X
(b)	The were no visible signs of material failure on the wheelchair securing points	X
(c)	There were no components, fragments or accessories of the wheelchair with a mass of more than 100g that completely separated from the wheelchair	X
(d)	There were no fragmented or separated component, that may contact the occupant, produced with sharp edges less than radius 2 mm	X
(e)	There were no visible signs of failure on the wheelchairs primary load carrying components	X
(f)	There were no visible signs of failure on the wheelchairs seat adjusters	X
(g)	The ADT was removed from the wheelchair without the use of tools	X
(h)	The wheelchair was released from the tie-down system without the use of tools	X
(i)	The post test decrease of the mean H-point height is not more than 20%	X
(j)	Wheelchair and components did not cause partial or complete failure of the webbing of any of the WTORS assemblies during the test	X

The presented samples meet the requirements set out in the above mentioned standard.

### Test Laboratory:

Dahl Engineering - Research and Testing Laboratory  
Løvevej 3 - DK-7700 Thisted - Denmark  
Phone: 45 96180077 - Fax: 45 96180078  
e-mail: [Dahl@dahlengineering.dk](mailto:Dahl@dahlengineering.dk) – web page: [www.dahlengineering.dk](http://www.dahlengineering.dk)

Thisted 2. March 2018



Claus Dahl Pedersen  
Head of test laboratory

Test object: Medema mini crosser X model

Manufacturer: Medema Produktion A/S, Enggårdsvvej 7, DK-7400 Herning

Plotted graph and speed



**SLED - TEST**

Project: Medema mini crosser X-model

Editor: CDP

Date: 02/27/2018

File: Medema2018-026

Sensors: ASC 4311 400 g, S/N-Nr.:G 81289

Measurement: A/D Karte, DT 321

Analysis Sequence: Standard

Sled velocity: 48.9 km/h

Specification: ISO7176-19

Test type: Homologation Test

Test structure: Sled


Test sample: Medema mini crosser X-model

Comment to sample: w. Dahl 4 point HD WTORS

Occupant: HybridII 50% Male

General comment:

**SLED ACCELERATION**

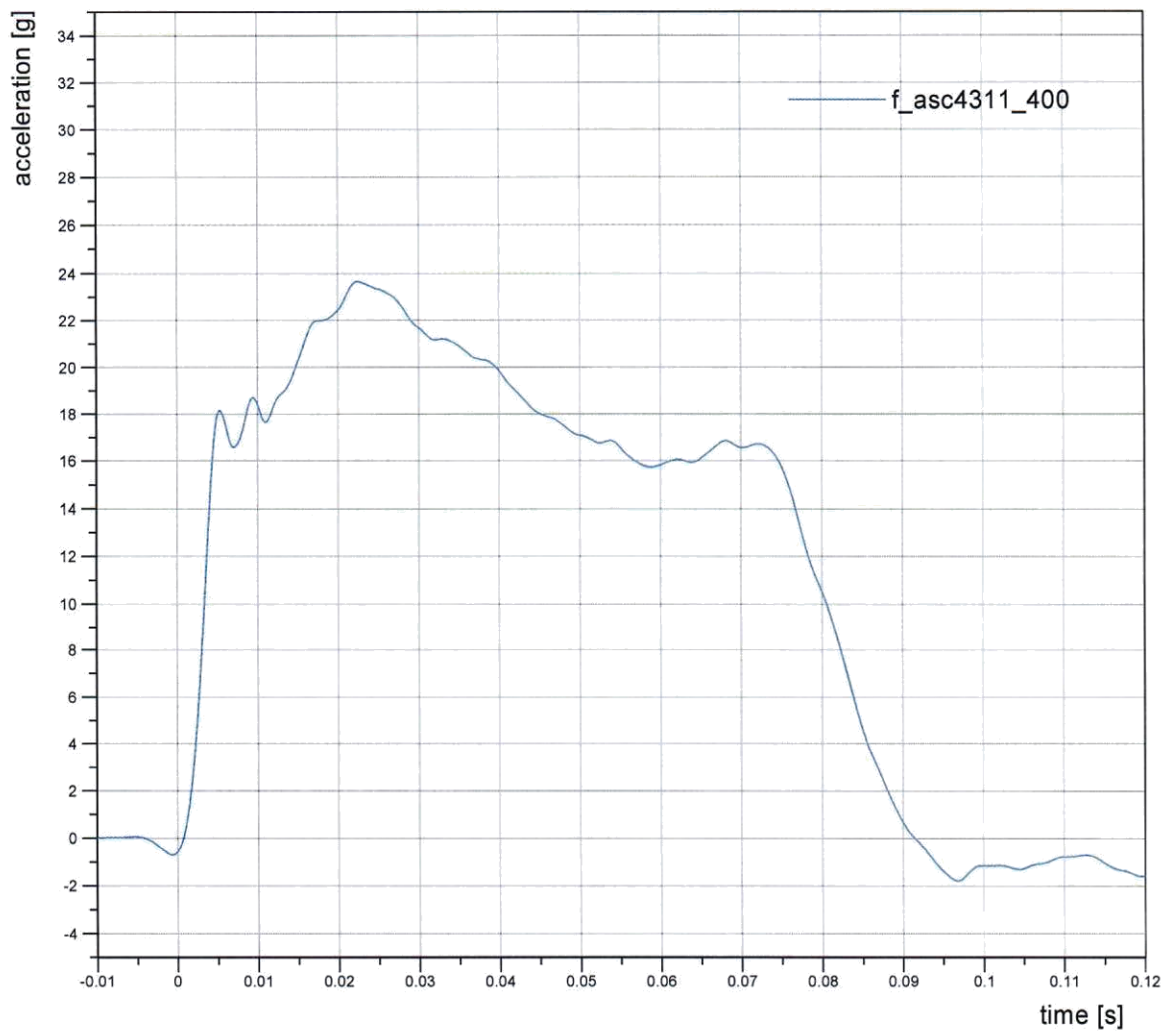

Pre- test photos



Post test photos

